INNOVATIVE TECHNOLOGY PRODUCTS CORP FOCUSED SHOCKWAVE

ITPC50001

CONTACT YOUR SALES REPRESENTATIVE EITHER IN FLORIDA OR CALIFORNIA










ITPC50001

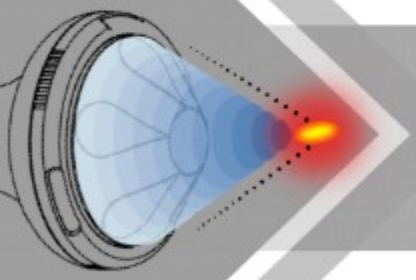




No.1	No.2	No.3	No.4	No.5	No.6	No.7





FOCUS SHOCKWAVES

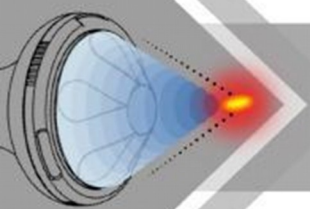



No.1	No.2	No.3	No.4	No.5	No.6	No.7

Welcome to the latest product from our company, the **ITPC50001 Focused Shock Wave Machine**.

The core technology of this system is an integrated piezoelectric shock wave source. The shock waves generated by this source are precisely focused and applied to the affected area for treatment. Silicone pad probes of different heights can be replaced to achieve multiple penetration depths, allowing direct access to the lesion site and ensuring both treatment depth and accuracy.

The ITPC focused shock wave system is a form of physical therapy. This therapy is safe, effective, non-invasive, precisely targeted, and offers deep tissue penetration. Therefore, it is also known as a “green therapy” and has been widely used as a preferred treatment for chronic pain, calcification, and tendon damage in the musculoskeletal system.

Before use, please read the instruction manual carefully and operate the device in accordance with the instructions.

The working principle is based on high-intensity focused shock wave energy generated by the device, which penetrates the skin surface and reaches specific deep tissues. This energy effectively stimulates the affected tissue, promotes the formation of new blood vessels, enhances blood circulation, and induces a controlled inflammatory response, thereby activating the body’s natural self-repair mechanisms.

In addition, the cavitation effect produced by focused shock waves generates vapor bubbles that rapidly collapse. This process helps break down adhesions, scar tissue, contractures, and blockages in damaged tendon areas, as well as calcified or fibrotic soft tissue. This is commonly referred to as “loosening” the injured area, which stimulates soft tissue regeneration, accelerates blood circulation, and promotes recovery.

At the same time, high-energy shock waves stimulate pain receptors and block the conduction of pain signals, achieving an immediate analgesic effect.

1. Cavitation Effect
When shock waves act on tissues, the gas within the tissues rapidly expands and collapses. During bubble collapse, a high-speed micro-jet phenomenon occurs, accompanied by rapid changes in bubble volume. This produces a cavitation effect, which can cause microcapillary rupture, release of cellular components, and generation of free radicals. These processes stimulate new blood vessel formation, help clear occluded micro vessels, accelerate microcirculation at the treatment site, improve local blood flow, and reduce adhesion in soft tissues.

---

2. Piezoelectric Effect
As a mechanical force, shock waves act on bone tissue by increasing internal stress and generating polarization potential, resulting in a piezoelectric effect. This process accelerates healing, promotes collagen production, enhances metabolism and microcirculation, and supports the formation of new blood vessels in ligaments. It also stimulates the proliferation and differentiation of osteoblasts, thereby promoting bone regeneration and healing.

---

3. Metabolic Activation Effect
By acting on localized diseased tissues, shock waves increase blood supply and deliver growth factors to the affected area. This stimulates stem cell transformation into normal tissue structures, reduces inflammation and edema, and accelerates the overall recovery process.

---

4. Analgesic Effect
High-intensity shock waves strongly stimulate nerve endings, reducing nerve sensitivity and inhibiting the transmission of pain signals. At the same time, biochemical changes around the cells promote the release of substances that suppress pain and increase the pain threshold, thereby providing effective pain relief.

shock wave

1. Application in Orthopedics
The ITPC focused shock wave machine has a wide range of applications in orthopedics. It is primarily used for the rehabilitation of fractures and bone cracks following surgery, as well as for the treatment of arthritis and ligament injuries.

Shock wave therapy delivers high-pressure energy that penetrates deep tissues, effectively promoting the repair and regeneration of bones and joints. For patients who require faster recovery, this technology provides a highly effective and efficient treatment option.

---


2. Application in Sports Medicine
In the field of sports medicine, focused shock wave machines are widely used for treating sports injuries and enhancing athletic performance. By promoting tissue repair and improving blood circulation, the system helps athletes recover more quickly while also supporting performance improvement.

Shock wave therapy is especially suitable for athletes who need to return to activity in a short period of time, enabling faster recovery from injuries and a quicker return to high-intensity performance.

---

3. Application in Neurology and Rehabilitation Medicine
The focused shock wave machine also plays an important role in neurology and rehabilitation medicine. It has been proven effective in relieving chronic pain and supporting the recovery of nerve damage.

Shock wave therapy stimulates body tissues, enhances blood circulation, and promotes nerve repair. For patients requiring long-term rehabilitation and pain management, it provides a comprehensive and effective treatment solution.

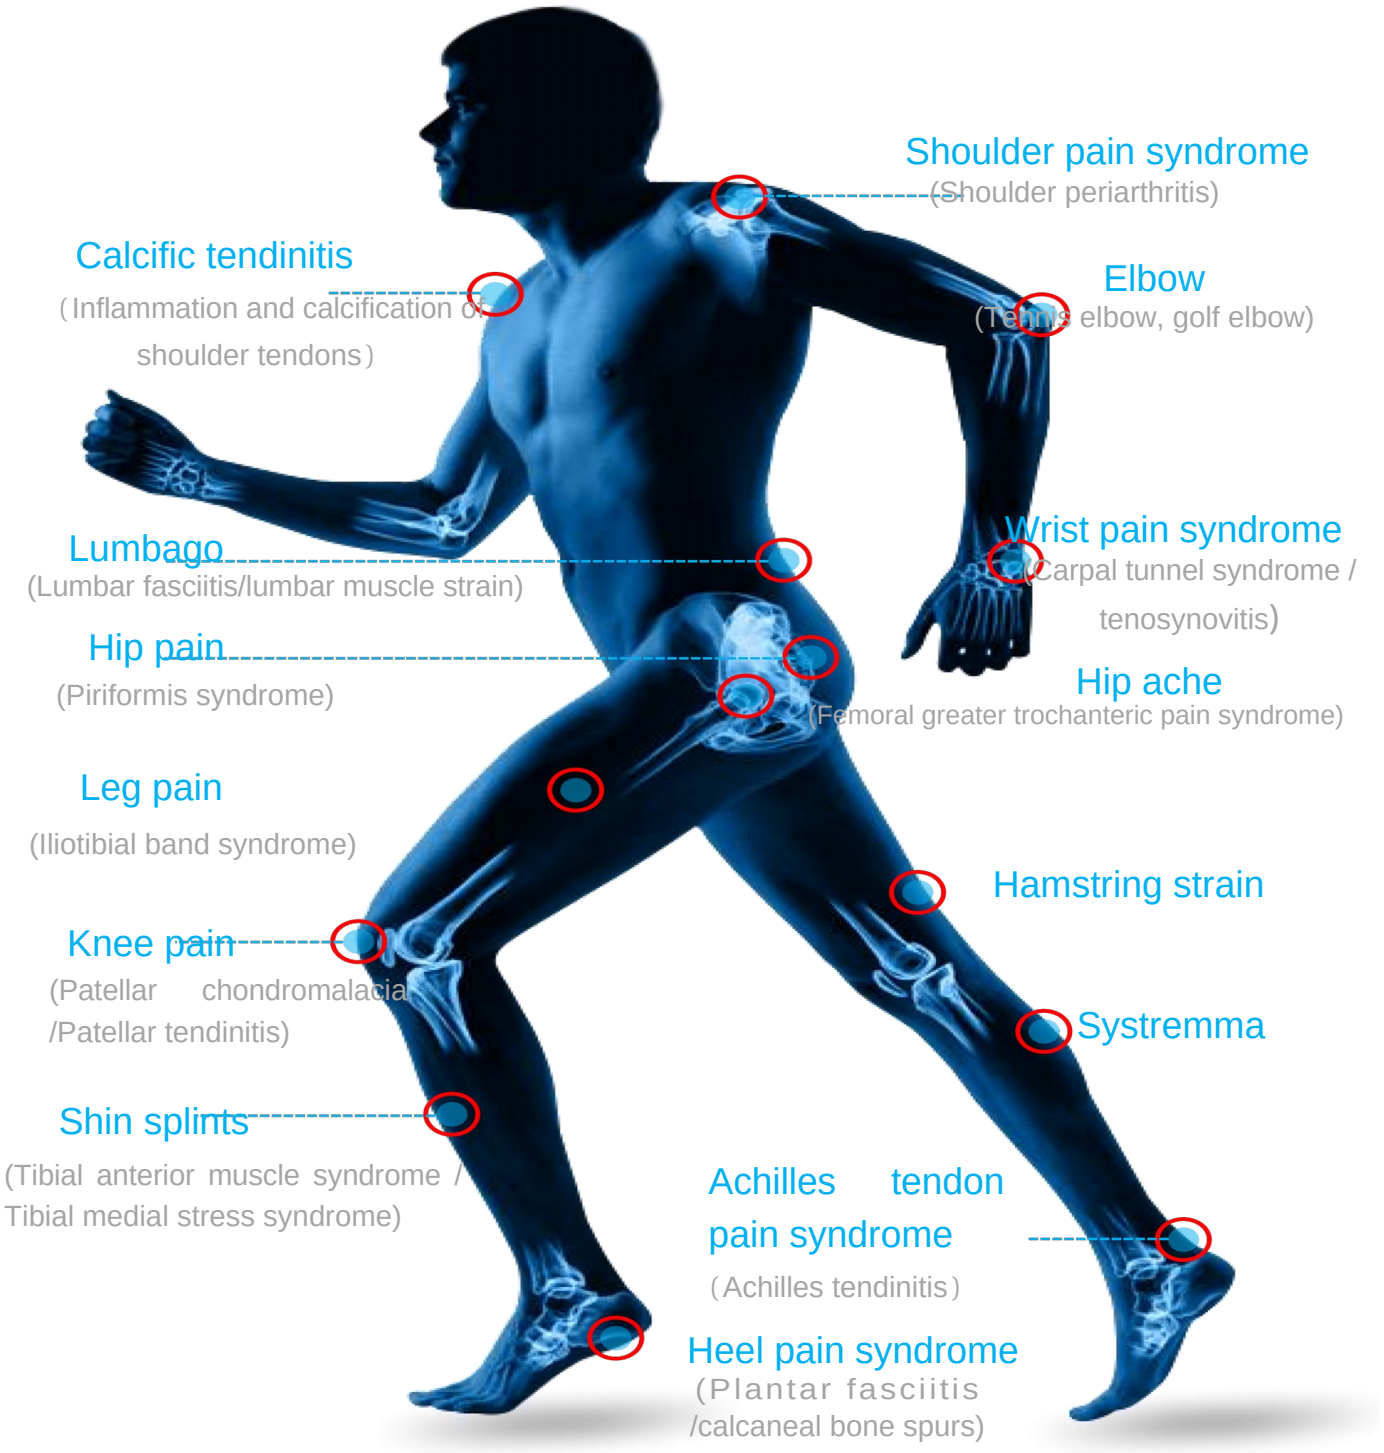
Shoulder pain syndrome
(Shoulder periarthritis)
Calcific tendinitis
（Inflammation and calcification of shoulder tendons）
Elbow
(Tennis elbow, golf elbow)
Lumbago
(Lumbar fasciitis/lumbar muscle strain)
Wrist pain syndrome
(Carpal tunnel syndrome / tenosynovitis)
Hip pain
(Piriformis syndrome)
Hip ache
(Femoral greater trochanteric pain syndrome)
Leg pain
(Iliotibial band syndrome)
Hamstring strain
Knee pain
(Patellar chondromalacia /Patellar tendinitis)
Systremma
Shin splints
(Tibial anterior muscle syndrome / Tibial medial stress syndrome)
Achilles tendon pain syndrome
（Achilles tendinitis）
Heel pain syndrome
(Plantar fasciitis /calcaneal bone spurs)

Key Features & Advantages

1. Intelligent Operation with User-Centered Design
The ergonomic handpiece features a **1.8-inch integrated display**, allowing real-time control and parameter adjustment directly from the device. This significantly enhances operational efficiency and ease of use for practitioners.

2. Precision Control with Variable Focusing
Equipped with **7 interchangeable silicone probe pads**, the system enables highly accurate control of penetration depth. This ensures targeted treatment across varying tissue depths, addressing a wide range of clinical conditions.

3. Deep Penetration with Flexible Coverage
By utilizing probes of different heights, the device allows **customizable shockwave depth and focus range**. Its strong penetration capability ensures effective treatment of both superficial and deep tissues, expanding overall therapeutic versatility.

4. Non-Invasive Treatment – No Downtime
EMIMPACTPOE focused shockwave therapy is **completely non-surgical**, requiring no incisions or injections. Patients experience minimal discomfort and can resume normal activities immediately, improving overall satisfaction and recovery speed.

5. Proven Safety and Clinical Effectiveness
This technology eliminates many risks associated with traditional surgical procedures. It offers a **safer, low-risk alternative** while maintaining high therapeutic effectiveness.

6. Eco-Friendly "Green Therapy"
Recognized as a **modern green treatment solution**, this therapy aligns with today's medical standards by delivering **low-impact, high-efficiency outcomes** without pharmaceuticals or invasive intervention.

7. Comfortable Treatment Experience
Despite delivering high peak pressure at the focal point, the system is designed with a **wide wave-source aperture**, ensuring low energy density at the skin surface. This results in a **comfortable, virtually painless experience** for patients.

Additional Features & Patient Benefits

7. Comfortable, Low-Pain Treatment Experience
While delivering high peak pressure at the focal point, the system maintains **low energy density at the skin surface**. This significantly reduces surface discomfort and minimizes the risk of tissue pain, ensuring a more comfortable patient experience.

8. Ultra-Quiet, Low-Noise Operation
Unlike traditional pneumatic ballistic or other focused shockwave systems that can generate significant noise, this device utilizes **advanced piezoelectric focusing technology with anti-hemispherical surface integration**. The result is a **stable, low-**

noise, vibration-free treatment environment, enhancing patient comfort and clinical experience.

9. Fast and Efficient Treatment Sessions

Each session typically lasts **10–15 minutes**, delivering **rapid therapeutic effects** while maintaining a high le

Safety Guidelines & Operating Precautions

1. Proper Grounding Requirement

Always use a power plug with a **grounding pin**, and ensure the power outlet is properly grounded to prevent electrical hazards.

2. Correct Power Supply

Verify that the power supply matches the **specified voltage indicated on the device**. Incorrect voltage may cause malfunction or permanent damage to internal components.

3. Stable Electrical Input

Ensure a **stable and reliable power source**. In areas with voltage fluctuations, the use of a **regulated power supply** is strongly recommended.

4. Use Approved Accessories Only

To maintain optimal performance and extend the device's lifespan, use only **manufacturer-approved or recommended accessories**.

5. Adequate Ventilation

Position the device at least **30 cm away from walls or obstructions** to allow proper heat dissipation and prevent overheating.

6. Environmental Conditions

Avoid placing the device in **high-temperature or high-humidity environments**, as this may affect performance and durability.

7. Touchscreen Handling

The system features a **capacitive touchscreen**. Operate it using your fingertip only—**do not use sharp or hard objects** to prevent damage.

8. Accessory Care & Maintenance

All accessories are **precision components**. Handle and maintain them carefully during and after use to avoid premature wear or failure.

9. Cleaning Precautions

Do not use **alcohol or corrosive cleaning agents** on the main unit or handpiece, as they may damage surfaces and internal components.

10. Post-Use Cleaning

After each use, clean accessories with **water or normal saline**, then dry thoroughly with a soft, dry cloth.

11. Handle with Care
Avoid dropping or striking the handpiece and accessories. **Damage caused by improper handling is not covered under warranty**.

12. Patient Safety
Ensure that the patient is **not in contact with metal objects or alternative grounding paths** during operation.

13. Pre-Use Inspection
Before each session, inspect the device and all accessories, especially **cables and connectors**—for any signs of damage.

14. Power Down After Use
When not in use, **turn off the device**, unplug it, and store all accessories properly. Use a **dust cover** when available.

15. No Unauthorized Modifications
Do not disassemble or modify the device without authorization. Unauthorized changes may compromise safety and void warranty.

16. Fault Handling
If any malfunction occurs, **stop using the device immediately** and contact authorized support for assistance.

vel of comfort and convenience for both patients and practitioners.

Warranty Policy & Package Contents

Warranty Coverage

- **Main Unit (Host):** 1-Year Limited Warranty
- **Accessories:** 3-Month Limited Warranty

1. Warranty Terms

- The warranty period begins from the **date of shipment from the factory**.
- During the warranty period, any **malfunction or failure not caused by human factors** will be repaired **free of charge**.

2. Warranty Exclusions

The warranty does **not** cover damage or faults resulting from:

- **Unauthorized servicing**, disassembly, or modification
- **Improper use**, accidental drops, or physical impact
- Use of **non-original or non-approved parts and accessories**
- **Natural disasters** or force majeure events (e.g., fire, flood, power surges)

Standard Package Contents

Item	Quantity
Main Unit (Host)	1 pc
Handle	1 pc
Silicone Pads	7 pcs
Hangers	2 pcs
Power Cable	1 pc

Technical Specifications

Product Name:
ITPC50001

Touch Screen:
Toughened glass capacitive touch screen, 15 inches

Penetration Depth:
4 ~ 66 mm

Pulse Frequency:
1 ~ 10 Hz

Strength Grade:
1 ~ 8 Bar

Operating Voltage:
AC 100V ~ 240V, 50Hz – 60Hz

Power:
10 – 500 W

Air Box Size:
53 × 50 × 60 cm

Gross Weight:
23 kg

Device Dimensions

- Height: **17.3 in** (44 cm)
- Width: **15.4 in** (39 cm)
- Depth: **16.0 in** (40.5 cm)

Packaging Box Dimensions

- Height: **23.6 in** (60 cm)
- Width: **19.7 in** (50 cm)
- Depth: **20.9 in** (53 cm)


Note:

Installation & Setup

1. Installation Steps


- Install the **hanger** onto the device.
- Connect the **handle** to the designated socket on the back of the device.
- Ensure proper alignment, then securely insert the handle and place it into the hanger.
- **2. Power Connection**

- Insert the **power cord** into the power socket located at the rear of the device.
- Turn on the main power supply, then switch on the device.
- The system will **start up immediately**.

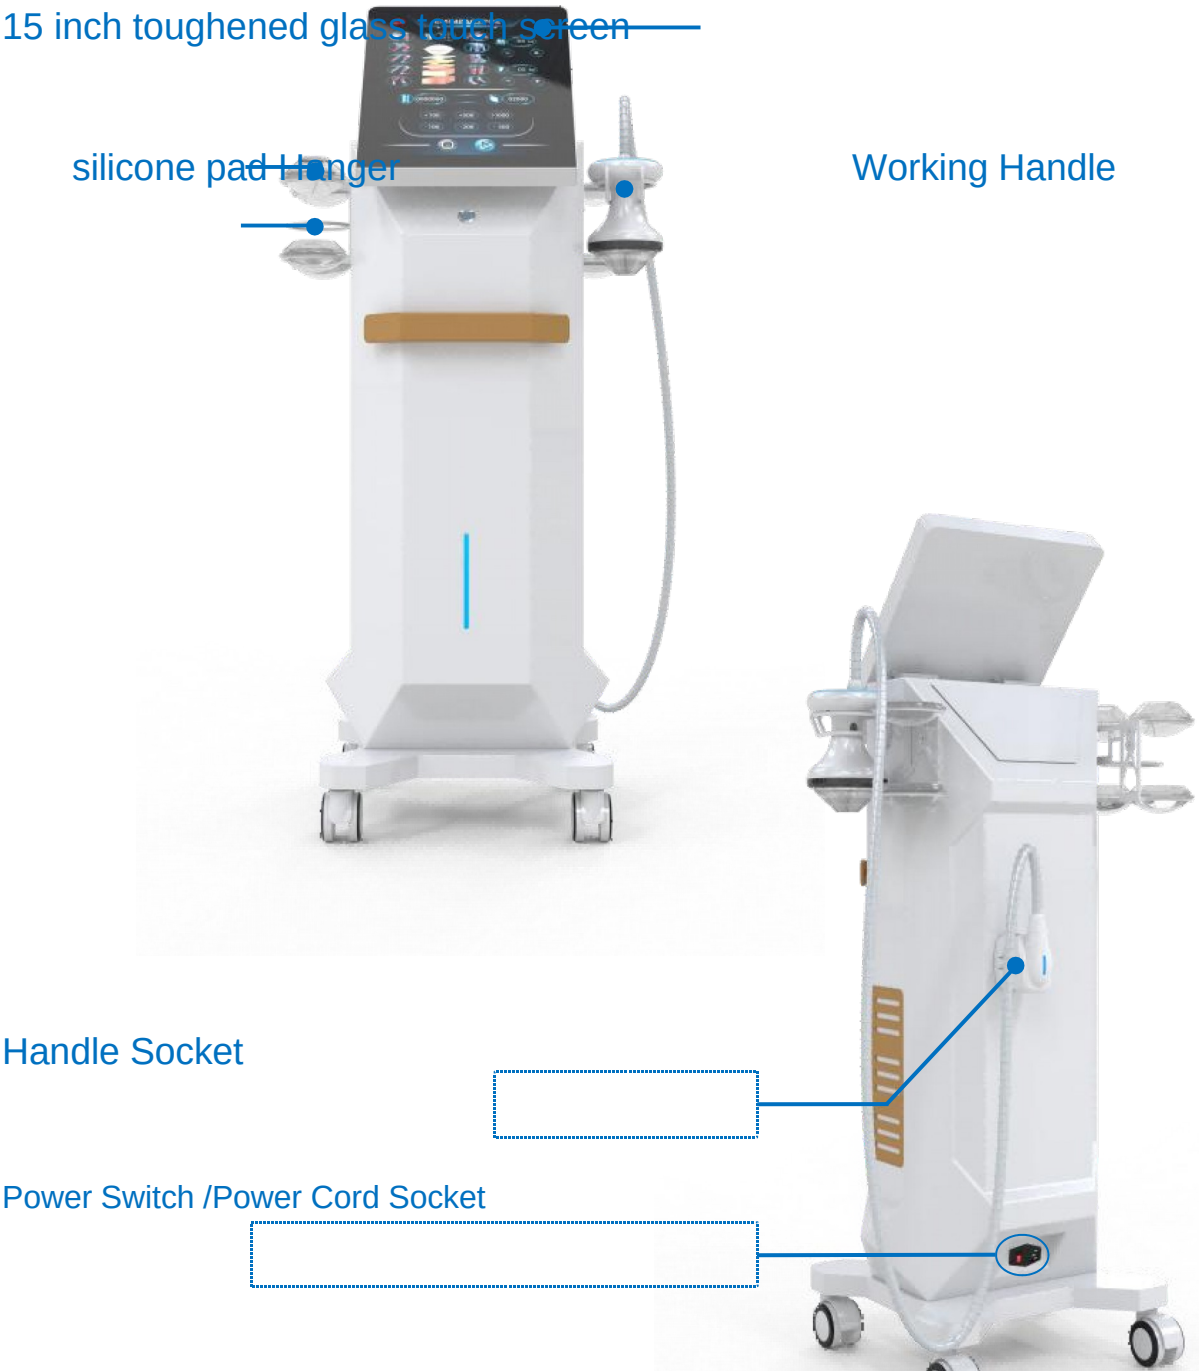

Accessory Instructions

- The **penetration depth of the shock waves** can be adjusted using the **distance device (gel pad)**. By installing the appropriate gel pad, the focusing depth can be precisely aligned with the target treatment area.
- The system includes **7 interchangeable silicone pads**, providing adjustable penetration depths ranging from **4 mm to 66 mm**. This allows practitioners to select the appropriate depth based on the specific treatment area and patient needs.

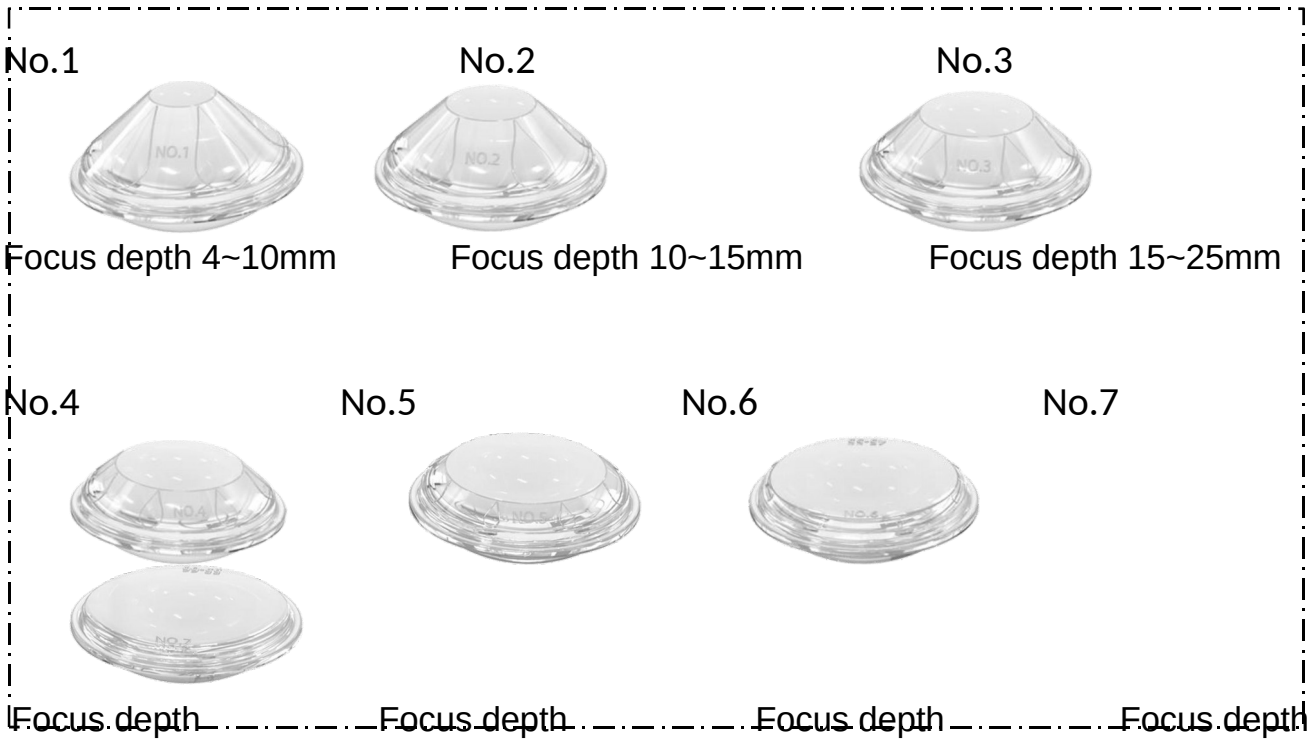


Gel Pad Usage & Maintenance Guidelines

- **Inspection & Replacement**
  If the gel pad shows visible changes such as **discoloration, loss of luster, cracks, bubbles, surface deformation, or leakage at connection points**, it must be replaced immediately.
- **Routine Condition Checks**
  Regularly inspect the gel pad for **cracks or surface damage**. Any sign of deterioration requires prompt replacement to ensure safe and effective operation.
- **Treatment Depth Selection**
  For applications such as **enhancing skin elasticity and stimulating collagen production**, or targeting **fat cell membrane disruption**, use a **shallower-depth gel pad** for optimal results.
- **Depth Calibration for Fat Treatment**
  Measure the treatment area using a **manual fat measurement tool**, then select

and install a gel pad with a depth set to approximately **50% of the measured thickness** for accurate targeting

• **Installation is as shown in the following figure:**

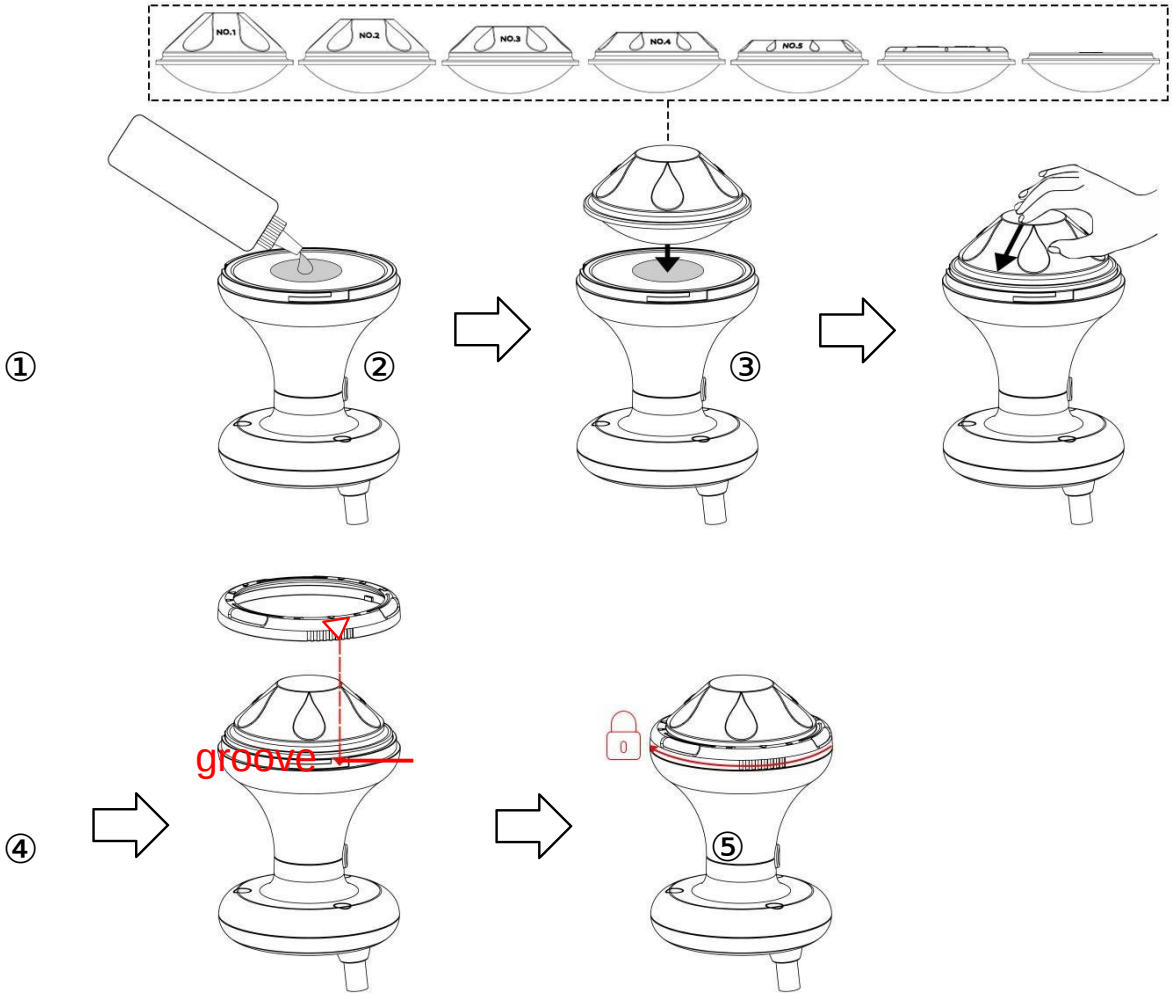

Silicone Head Installation & Gel Application

- **Step 1 (Figure ①): Apply Contact Gel**
  Apply a **sufficient amount of contact gel** to the handle.
  Note: Do not operate the device without gel, and avoid using too little, as this may affect performance (incorrect usage shown in Figure ⑥).
- **Step 2 (Figure ②): Select Silicone Connector**
  Choose the appropriate **silicone connector** based on the required **treatment depth and focal penetration**.
- **Step 3 (Figure ③): Attach Silicone Head**
  Insert the silicone head and press gently to ensure **full contact with the handle**.
  Rotate it slightly to **eliminate air bubbles**. If bubbles remain, apply additional gel to improve contact.

- **Step 4 (Figure ④): Install Locking Ring**
  Align the silicone head with the groove, then install the **locking ring (fixing ring)** securely.
- **Step 5 (Figure ⑤): Secure the Assembly**
  Rotate the locking ring **clockwise** until the silicone head is firmly secured in place.

- As shown in Figure ⑥ below: Schematic diagram of incorrect installation.

⑥



- As shown in Figure ⑦ below: Schematic diagram of correct installation.

⑦




Important Note

After installing the silicone head, ensure that **no air bubbles are present underneath**.
If air bubbles are detected, gently rotate the silicone head to eliminate them.

Once proper contact is achieved, install the **locking ring cover** and rotate it **clockwise** to securely fasten the silicone head in place.

Touchscreen Button Functions & Overview

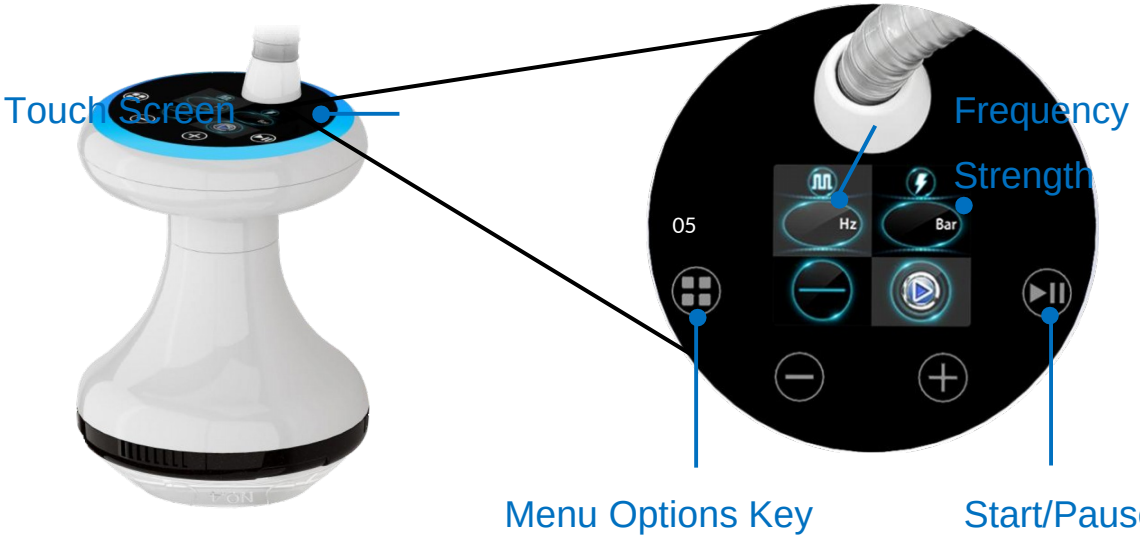

Menu option key description: Allow users to touch and click th menu option

key to control the frequency and intensity of the two windows to switch back and forth. When the desired window is selected, the number turns blue, and users can click to adjust para ers.

Operation/Stop button



The introduction of the work button in Figure 2 is as follows:

• Click【  】Indicates returning to the previous interface.

• 【 

】：Impact counter, record the total number of occurrences.

• 【 

】：You can customize the preset number of shockwaves strikes, click【+】【-】to adjust by adding or subtracting.

【 

：This key increments the preset number of shock waves in units of +100 each time.

【 

：This key increments the preset number of shock waves in units of +500 each time.

【 

：This key increments the preset number of shock waves in units of +1000 each time.

【 

】：This key decreases in units of -100 each time.

【 

】：This key decreases in units of -200 each time.

【 

】：This key decreases in units of -500 each time.

• 【 

】：Frequency, representing the speed of shock wave output, ranging from 1-10Hz, with increments of 1 per level. Click【+】【-】to adjust by adding or subtracting.

The frequency of treatment depends on individual tolerance and tissue response.

• 【 

: Intensity, range 1-10Bar, increments of 1 per level, click 【+】【-】to adjust by adding or subtracting.


It is necessary to start treatment at the lowest intensity and gradually increase the treatment intensity according to the user's feelings.

• Clicking on【  】to turn it into【  】indicates that the device is started and ready, and the controller operation key needs to be pressed to start working and outputting energy.


• Click【  】turn into【  】Indicates pause and put the device in standby state.

---


3. In the working interface of Figure 2, taking the hand as an example, the following is introduced: click “  select part Icon “  then long press the part icon “  for 3 seconds to pop up the corresponding help window for the current part. You can press “  to close the help window.

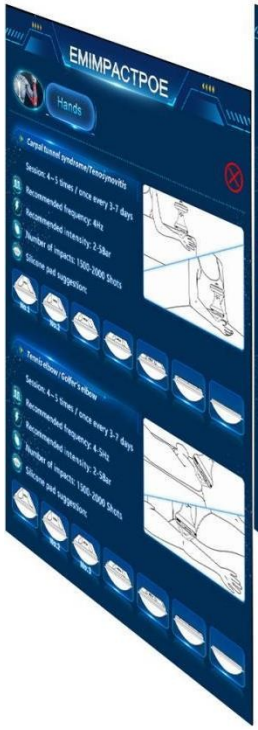
EMIMPACTPOE
Hands
Carpal tunnel syndrome/Tenosynovitis
Session: 4~5 times / once every 3~7 days
Recommended frequency: 4Hz
Recommended intensity: 2-5Bar
Number of impacts: 1500-2000 Shots
Silicone pad suggestion:
Tenicritis/Golfer'sElbow
Session: 4~5 times / once every 3~7 days
Recommended frequency: 4-5Hz
Recommended intensity: 2-5Bar
Number of impacts: 1500-2000 Shots
Silicone pad suggestion:


EMIMPACTPOE
Knee
Patellar chondromalacia / Patellar tendinitis
Session: 4~5 times / once every 3~7 days
Recommended frequency: 4Hz
Recommended intensity: 2-5Bar
Number of impacts: 1500-2000 Shots
Silicone pad suggestion:

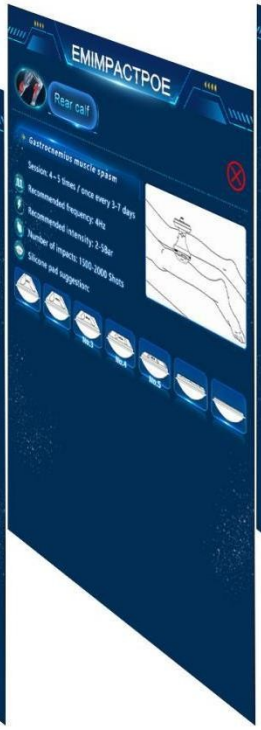
EMIMPACTPOE
Rear calf
Gastrocnemius muscle spasm
Session: 4~5 times / once every 3~7 days
Recommended frequency: 4Hz
Recommended intensity: 2-5Bar
Number of impacts: 1500-2000 Shots
Silicone pad suggestion:


EMIMPACTPOE
Front calf
Tibial anterior muscle syndrome
Session: 4~5 times / once every 3~7 days
Recommended frequency: 4Hz
Recommended intensity: 2-5Bar
Number of impacts: 1500-2000 Shots
Silicone pad suggestion:

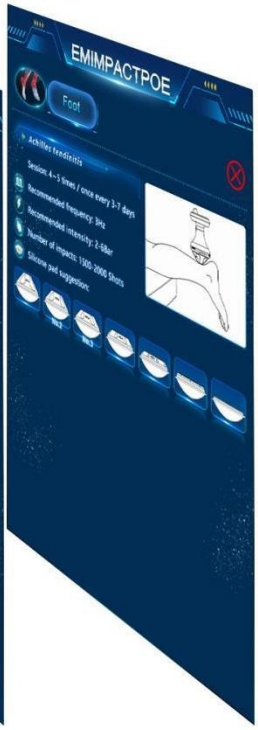
EMIMPACTPOE
Foot
Achilles tendinitis
Session: 4~5 times / once every 3~7 days
Recommended frequency: 3Hz
Recommended intensity: 2-5Bar
Number of impacts: 1500-2000 Shots
Silicone pad suggestion:


EMIMPACTPOE
Shoulder
Calcific tendinitis
Session: 4~5 times / once every 3~7 days
Recommended frequency: 4-5Hz
Recommended intensity: 4-7Bar
Number of impacts: 1500-2000 Shots
Silicone pad suggestion:
Scapulohumeral periarthritis
Session: 4~5 times / once every 3~7 days
Recommended frequency: 4Hz
Recommended intensity: 2-5Bar
Number of impacts: 1500-2000 Shots
Silicone pad suggestion:


EMIMPACTPOE
Waist Back
Lumbago fasciitis / lumbar muscle strain
Session: 4~5 times / once every 3~7 days
Recommended frequency: 4Hz
Recommended intensity: 2-5Bar
Number of impacts: 1500-2000 Shots
Silicone pad suggestion:


EMIMPACTPOE
Hip
Greatertrochanteric pain syndrome (GTPS)
Session: 4~5 times / once every 3~7 days
Recommended frequency: 4-5Hz
Recommended intensity: 2-5Bar
Number of impacts: 1500-2000 Shots
Silicone pad suggestion:
Piriformis syndrome
Session: 4~5 times / once every 3~7 days
Recommended frequency: 4-5Hz
Recommended intensity: 2-5Bar
Number of impacts: 1500-2000 Shots
Silicone pad suggestion:


EMIMPACTPOE
Thigh
Iliotibial band syndrome
Session: 4~5 times / once every 3~7 days
Recommended frequency: 4Hz
Recommended intensity: 2-5Bar
Number of impacts: 1500-2000 Shots
Silicone pad suggestion:
Hamstring strain
Session: 4~5 times / once every 3~7 days
Recommended frequency: 4Hz
Recommended intensity: 2-5Bar
Number of impacts: 1500-2000 Shots
Silicone pad suggestion:


EMIMPACTPOE
Foot sole
Plantar fasciitis
Session: 4~5 times / once every 3~7 days
Recommended frequency: 4Hz
Recommended intensity: 3-7Bar
Number of impacts: 1500-2000 Shots
Silicone pad suggestion:
Calcaneal bone spur
Session: 4~5 times / once every 3~7 days
Recommended frequency: 4-5Hz
Recommended intensity: 4-7Bar
Number of impacts: 1500-2000 Shots
Silicone pad suggestion:

Treatment Settings Reference & Clinical Protocol

setting

ITPC Recommended Treatment Ranges & Parameter Settings

Surgical site	silicone pad	Number of impacts	Frequency (Hz)	Intensity (Bar)
Shoulder (Calcium area of aponeurosis)	No.4、No.5、No.6	1500~2000 Shots	4~5Hz	4~7
Scapulohumeral periarthritis	No.4、No.5、No.6	1500~2000 Shots	4Hz	3~5
Elbow (Tennis elbow, Golfer's elbow)	No.2、No.3	1500~2000 Shots	4~5Hz	2~5
Wrist (carpal tunnel syndrome / tenosynovitis/TFCC syndrome)	No.1、No.2	1500~2000 Shots	4Hz	2~5
Thigh (iliotibial band syndrome/hamstring strain)	No.5、No.6、No.7	1500~2000 Shots	4Hz	2~5
Knee (Patellar chondromalacia / Patellar tendinitis)	No.2、No.3	1500~2000 Shots	4Hz	2~5
Front calf (Tibial anterior muscle syndrome /Tibial medial stress syndrome)	No.1、No.2	1500~2000 Shots	4Hz	2~5
Rear calf (Gastrocnemius muscle spasm)	No.3、No.4、No.5	1500~2000 Shots	4Hz	2~5
Foot (Achilles tendinitis)	No.2、No.3	1500~2000 Shots	3Hz	2~6
Foot (Calcaneal bone spur)	No.3、No.4	1500~2000 Shots	4~5Hz	4~7
Foot sole Plantar fasciitis	No.2、No.3、No.4	1500~2000 Shots	4Hz	3~7

Contraindications & Safety Precautions

Do NOT perform treatment under the following conditions:

- During **menstruation, pregnancy, or lactation**
- Patients with **hemophilia** or those undergoing **anticoagulant therapy**
- Presence of **thromboembolic conditions**
- **Children with developing or immature bones**
- Areas with **surgical wounds, skin damage, abrasions, open lesions, acute inflammation, or infection**
- Patients with **contagious or legally notifiable infectious diseases**
- Patients who have received **corticosteroid injections or X-ray therapy within the past 6 weeks** *(use with caution)*
- Individuals with **long-term steroid use** or conditions causing **telangiectasia** (e.g., liver dysfunction)
- Patients with serious conditions such as:
  - **Malignant tumors / cancer**
  - **Epilepsy**
  - **Uncontrolled hypertension**
  - **Polyneuropathy**
- Any **unstable medical or psychiatric condition**

Do NOT apply treatment to the following areas:

- **Sensitive or critical organs:**
  Eyes and surrounding areas, myocardium (heart), spinal cord, gonads (ovaries/testicles), kidneys, and liver
- **Air-filled organs or regions:**
  Lungs and intestines (due to cavitation effects of shock waves)
  - When treating near the back (lung region), penetration depth must be less than 20 mm
- **High-risk anatomical areas:**
  Large nerve bundles, major blood vessels, arteries, and areas near the **head and neck**
- **Areas with reduced or altered sensation**
- **Areas with implanted electronic or medical devices:**
  Such as **pacemakers, defibrillators, or nerve stimulators**
- **Areas with abnormal tissue growth:**
  Including both **benign and malignant proliferations**

Treatment Procedure

1. Identify Treatment Area
Determine the treatment area through **palpation**. Mark the area in advance to ensure **accurate targeting** during treatment.

2. Patient Positioning
Position the patient appropriately based on the treatment area. Ensure the patient is **comfortable** and the area is **fully accessible**.


3. Device Preparation
Select and install the appropriate **silicone pad probe**, preset the required parameters, and press the **Start button** to activate the device.


4. Apply Coupling Gel
Apply a sufficient amount of **coupling gel** to the treatment area. This ensures efficient transmission of shock waves.
Note: Operation without gel is strictly prohibited.

5. Begin Treatment
Place the silicone probe firmly against the treatment area, then press the **control button on the handle** to begin therapy.

6. Locate Trigger Points
Move the applicator slowly across the treatment area, making slight angle adjustments to identify and target **trigger points**.

7. Clinical Application Reference
Refer to treatment illustrations or examples for proper technique and positioning.

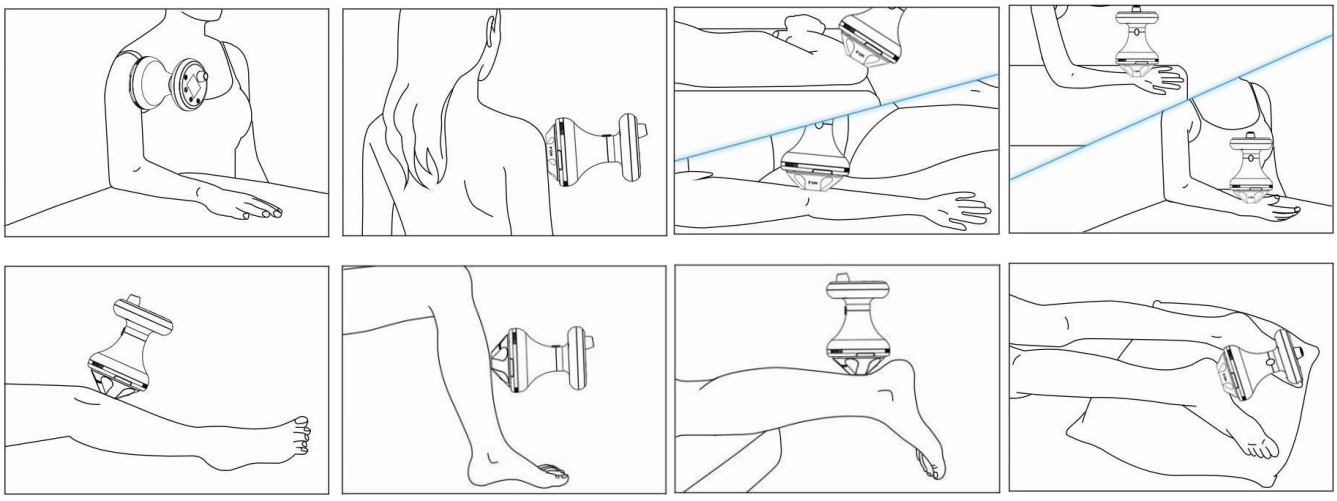

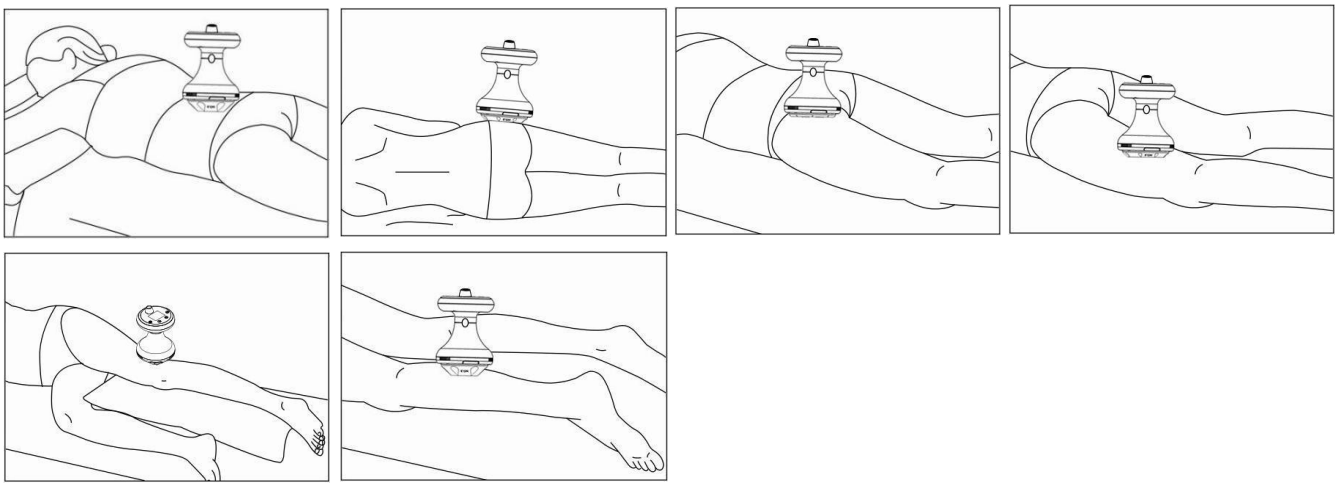

Treatment Completion & Post-Procedure Steps

8. Monitor and Adjust During Treatment
Perform the treatment according to the preset parameters. Continuously **monitor the patient's response** and adjust settings as needed or pause treatment if necessary.

- If the intensity is too high, adjust using either of the following methods:
  - **Reduce intensity level**
  - **Increasing frequency (speed)** higher frequency results in **lower impact force**

---

9. Post-Treatment Care
Once the session is complete and the preset number of pulses has been delivered:

- Remove any remaining **coupling gel** from the treatment area
- Assist the patient in returning to a **comfortable position**

---

10. Device Shutdown & Cleaning
After treatment:

- Turn off the device
- Remove the **handle locking ring** and take out the silicone pad
- Clean and wipe away any gel residue from both the **silicone pad and handle**

